


10/500230


1/2

FIG. 1

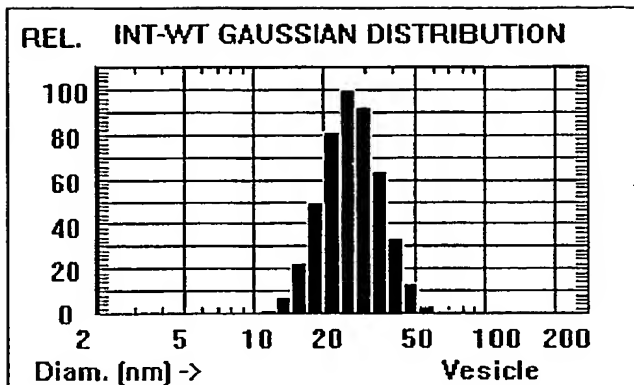

Intensity Weighting:
Mean Diameter = 27.5 nm
Std Deviation = 8.2 nm (29.7 %)

Cumulative Result:	Int-Wt	Vol-Wt
25 % of distribution <	19.8 nm	18.3 nm
50 % of distribution <	24.3 nm	22.4 nm
75 % of distribution <	29.6 nm	27.4 nm
90 % of distribution <	35.6 nm	33.0 nm
99 % of distribution <	47.9 nm	45.2 nm

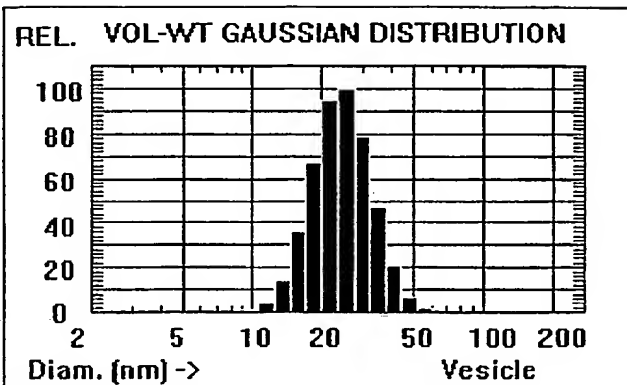


Volume Weighting:
Mean Diameter = 25.3 nm
Std Deviation = 7.5 nm (29.7 %)

Coeff. of Var'n = 0.297 Chi Sq. = 1.60
Baseline Adj. = 0.00 % Run Time = 0:10:5


BEST AVAILABLE COPY

2/2

FIG. 2

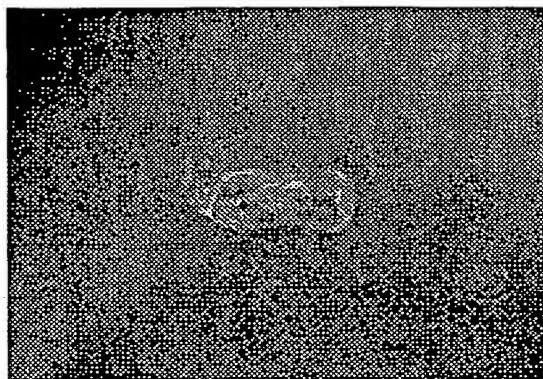

(A)

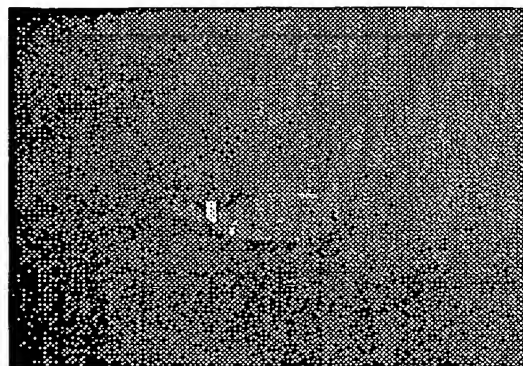

(B)

BEST AVAILABLE COPY